

Analysis	Standard Peptide Mass / Purity (HPLC-UV)
Client	Synerium

Sample


Selank 10mg
Synerium



RESULTS

VIAL	BATCH	PURITY	AMOUNT
#1 10mg	Sr-202601-036	99.78%	10.91 mg

#1 UV CHROMATOGRAM

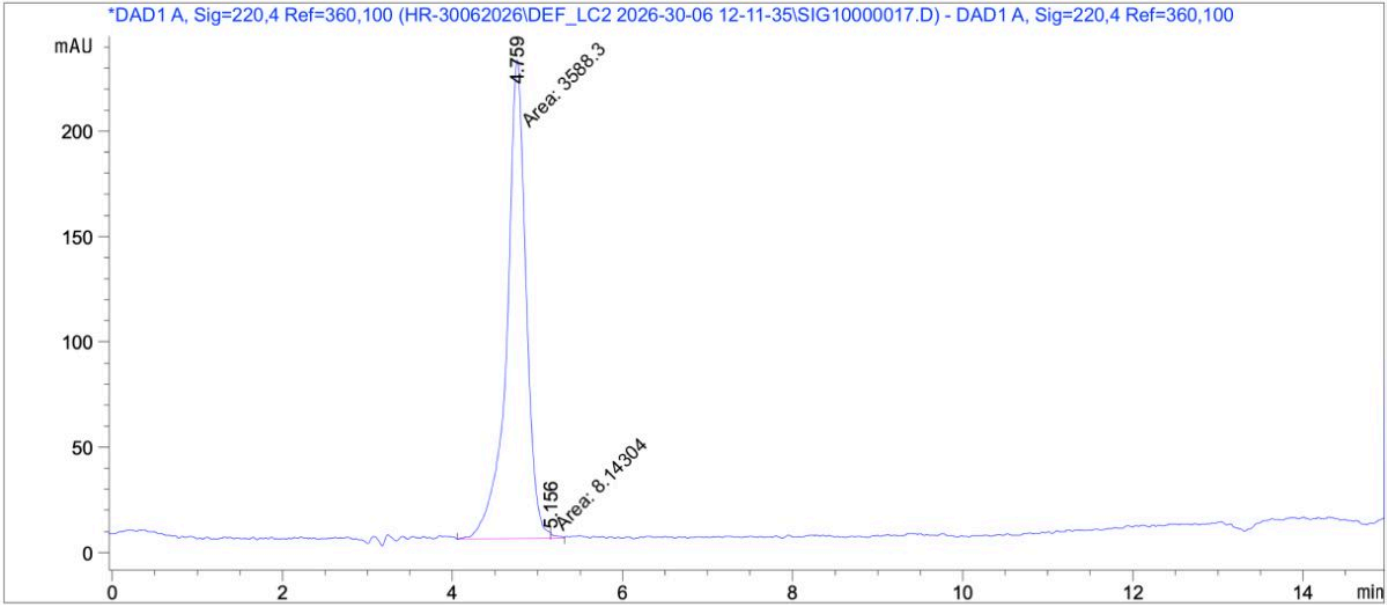

COMMENT

ANALYSIS CONDUCTED

30 JUN 2026

ZAGREB, CROATIA (EU)



Alex Mihaljcic

DIRECTOR

