



03 JUL 2026

|          |                                          |
|----------|------------------------------------------|
| Analysis | Standard Peptide Mass / Purity (HPLC-UV) |
| Client   | Synerium                                 |

## Sample


|            |
|------------|
| Semax 10mg |
| Synerium   |



## RESULTS

| VIAL    | BATCH         | PURITY | AMOUNT   |
|---------|---------------|--------|----------|
| #1 10mg | Sr-202601-039 | 99.18% | 10.44 mg |

## #1 UV CHROMATOGRAM

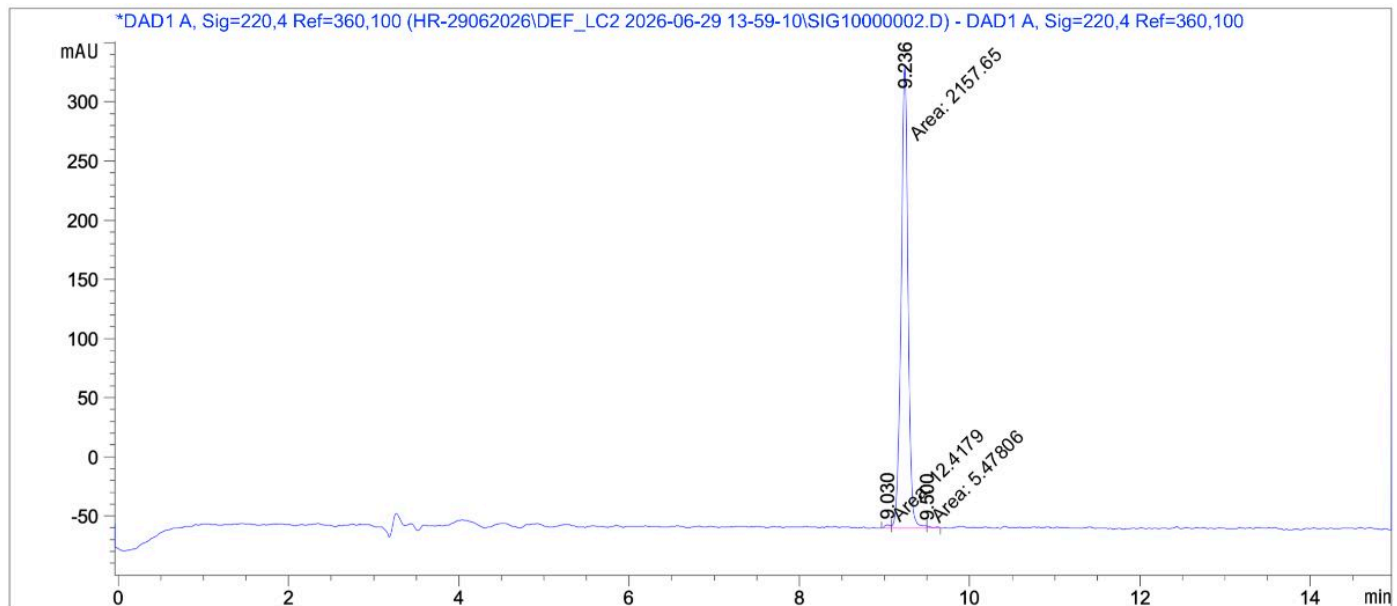

## COMMENT

## ANALYSIS CONDUCTED

29 JUN 2026

ZAGREB, CROATIA (EU)

Alex Mihaljcic  
DIRECTOR